

Medical Devices for Sleep Diagnostics and Therapy


# SOMNOmedics

## SOMNOwatch<sup>®</sup>


■ MINIMUM EFFORT

■ OPTIMUM DIAGNOSTICS


■ FLEXIBLE APPLICATION

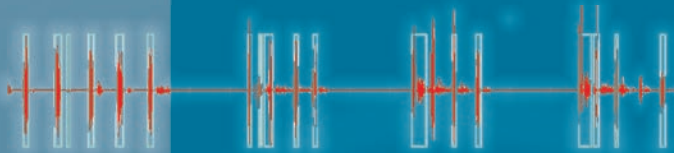

Respiration  
(Flow and Snore)

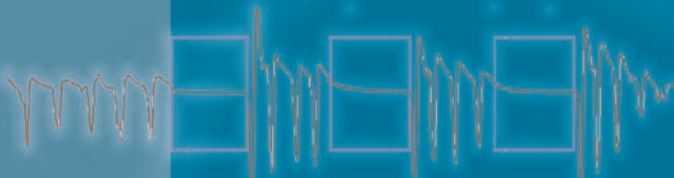

Tremor Analysis 3D

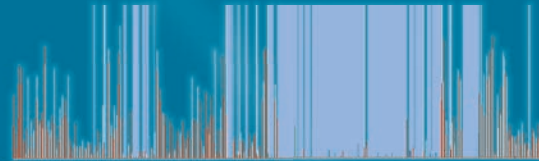

Actigraphy




PLM-Recorder



Sleep Profile  
(Wake, REM, 1, 2, 3, 4)



Long-term ECG Recording

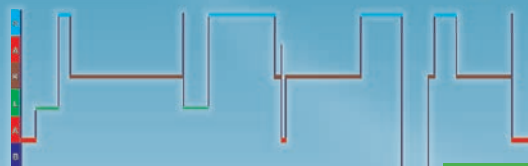

Body Position

## The All-rounder

FDA approved for adults only



# SOMNOwatch®

## Ambulatory Multi-Channel Monitoring


### Miniaturised - Mobile - Flexible

The rapid progression in electronics has led to a general miniaturisation in Mobile Medical Devices. The integration of multiple diagnostic functions into one single device allows for a flexible and cost effective system. **SOMNOwatch®** is a powerful miniaturised multi channel recorder which includes the comfort and user friendliness of a watch.

As a multi-channel system, the **SOMNOwatch®** can replace several common devices while providing excellent signal quality. **SOMNOwatch®** can be used for **Actigraphy** in order to determine Circadian Rhythm, **PLM detection**, **Tremor Analysis**, **Single Channel ECG** and **EEG recording**, **Body Temperature**, **Respiratory Screening** with Flow & Snoring, **Body Position**, and **Sleep/Wake Analysis**. The waterproof device is powered by a rechargeable Li-Ion battery and has an internal storage of 8/16 MB enabling long-term measurements of up to 26 days. Relevant points in time on the recording can easily be marked with the integrated Patient Marker.




**Exercise/Sport/Rehabilitation** - To get important Motor Activity performance information during Sport and Exercise, the **SOMNOwatch®** can be worn on the arm, leg, or body. Additionally, the **SOMNOwatch®** can measure ECG. The software synchronizes Heart Rate with Motor Activity. The correlation of Motor Activity and Cardiovascular Stress is very important for optimising and monitoring exercise and rehabilitation progress.

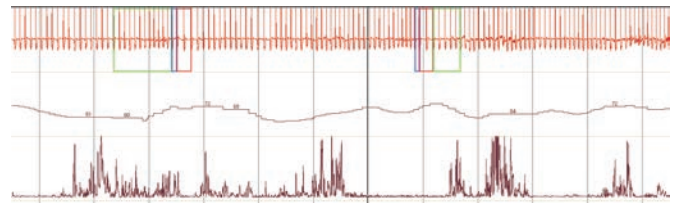




## PLM and RLS Recorder

Applied to the ankle, **SOMNOwatch®** can record Leg Movement continuously for up to 5 nights. It can differentiate between standing and lying using the integrated position sensor. With adjustable parameters, the software automatically recognises PLM movement patterns and evaluates the PLM index. By quantification of Motor Activity, RLS (Restless Legs) is rated. For an extended diagnosis, the EEG option can be added to provide EEG Derivation which can be used to provide the correlation of PLM's and Cortical Micro Arousals.



## Actigraphy

**Circadian Rhythm - SOMNOwatch®** is worn on the non-dominant arm for recording and objective recognition of the Sleep/Wake Rhythm. The activity is measured in epochs of 1 to 120 seconds and plotted as an Actigraphy Profile. The relevant measurement period (time in bed) is given using the integrated Light Sensor. As a result, disorders of the Circadian Rhythm e.g. for shift workers or pilots, can be documented. In Attention Deficit and Hyperactivity Disorder (ADHD), **SOMNOwatch®** can be used to diagnose and monitor the therapy of hyperactive children. Certain periods can be assigned to specific events, such as School, School Breaks and leisure time.

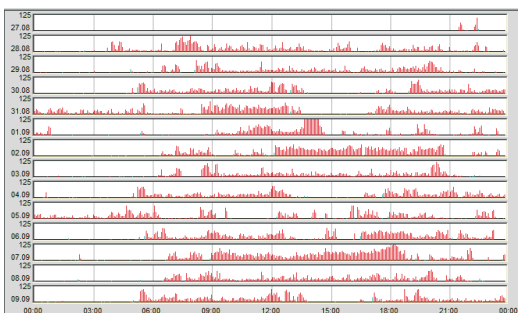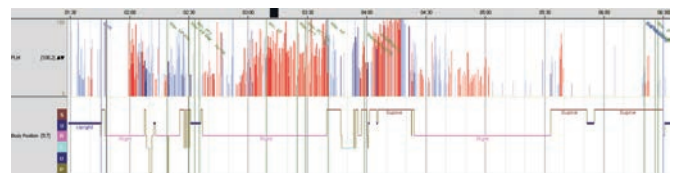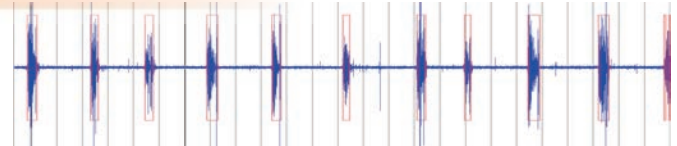

### Periodic Leg Movement (PLM)


	Sleep	REM	Non-REM	Wake	Total
Isolated-LMs (Index)	189 (45,0)	-	189 (45,0)	31 (544,5)	220 (51,7)
PLMs (Index)	235 (56,0)	-	235 (56,0)	22 (386,4)	257 (60,4)
Resp-LMs (Index)	14 (3,3)	-	14 (3,3)	1 (17,6)	15 (3,5)
Body Position -LMs (Index)	13 (3,1)	-	13 (3,1)	-	14 (3,3)
<b>PLMs with Micro Arousal</b>	<b>58 (13,8)</b>	-	<b>58 (13,8)</b>	<b>3 (52,7)</b>	<b>61 (14,3)</b>

### PLM Progression

Time	PLM
01:45 - 02:00	2 (8,32)
02:00 - 03:00	46 (46,00)
03:00 - 04:00	113 (113,00)
04:00 - 05:00	63 (63,00)
05:00 - 06:00	8 (8,00)
06:00 - 06:29	3 (6,02)



FDA approved for adults only







## Movement Analyser

The high frequency acquisition of movement enables **SOMNOWatch®** to make a very accurate frequency analysis using FFT. The recording of tremor intensity and tremor frequency can be achieved over a long period of time. This parameter can be used for the medical diagnosis and treatment of Parkinson's Disease.

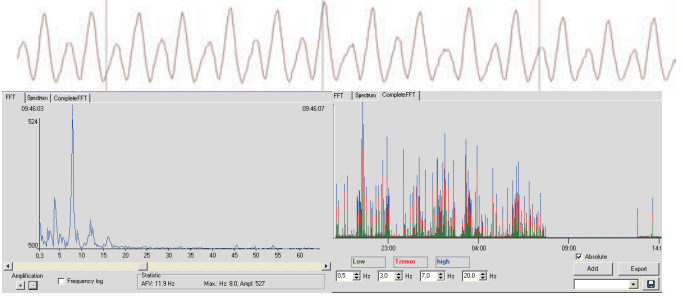


## Respiratory Screener

By using a combined sensor for Flow and Snore, the **SOMNOWatch®** can be used as a Respiratory Screener. Worn on the thorax, it can record Body Position, Acceleration, Light, Flow, and Snoring. The correlation of Body Position, Apnoea/Hypopnoea and Snoring can easily be detected. In addition to the diagnosis of Sleep Apnoea, the **SOMNOWatch®** can be used for recording patients connected to a CPAP machine.

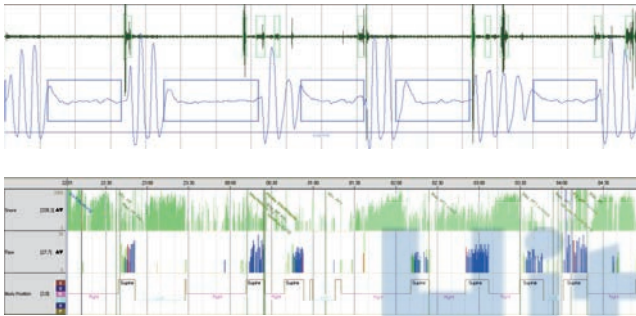

## Long-term ECG

**SOMNOWatch®** can store the raw data of a single channel ECG for up to 18 hours. The correlation between Heart Rate, its Rhythm, Actigraphy and Body Position gives very interesting information for the diagnosis and rehabilitation of Cardiovascular disease.

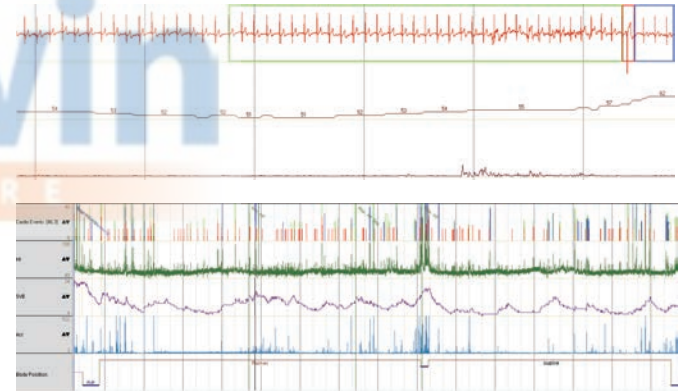


### Respiratory Analysis

Body Position	Prone	Supine	Left	Right	Upright
Sleep Time Fraction (%)	-	27,5	17,2	55,3	-
Total Events (Index)	-	171 (90,1)	7 (5,9)	13 (3,4)	-
Obstr. Apnoea (Index)	-	9 (4,7)	-	-	-
Central Apnoea (Index)	-	2 (1,1)	-	-	-
Mixed Apnoea (Index)	-	-	-	-	-
Hypopnoea (Index)	-	31 (16,3)	5 (4,2)	10 (2,6)	-
Flow Limitations (Index)	-	-	-	-	-

### Snore



	All	Prone	Supine	Left	Right	Upright
Snore (Index)	2335 (338,3)	-	387 (204,0)	328 (276,5)	1620 (424,2)	-
Absolute Snore (min)	42,1	-	5,4	6,2	30,5	-
Snore Episodes (min)	164,8	-	16,1	26,6	122,2	-
Snore epis. (% Sleep Time)	39,8					



## Sleep Recorder



In order to differentiate the sleep stages, the EEG option can be added to the Actigraphy of the **SOMNOWatch®**. The additional data allows for the differentiation of not only the Sleep/Wake Profile but also Wake, REM, 1, 2, 3 and Stage 4.

### Sleep Stages

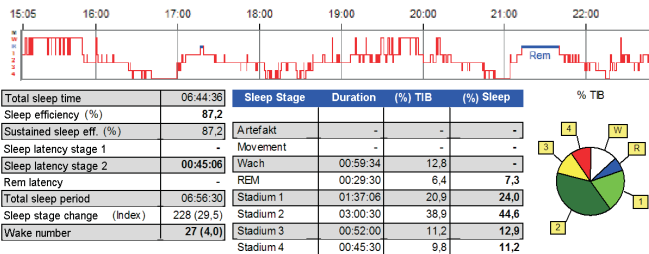

## Long-term EEG


With very little effort, the **SOMNOWatch®** can record a single channel EEG for up to 18 hours. The artefact identification is improved by the simultaneous measurement of Motor Activity. For an optimized analysis, the raw data is represented in the different EEG frequency bands. Spindles, K-complexes, and Micro Arousals are automatically scored.

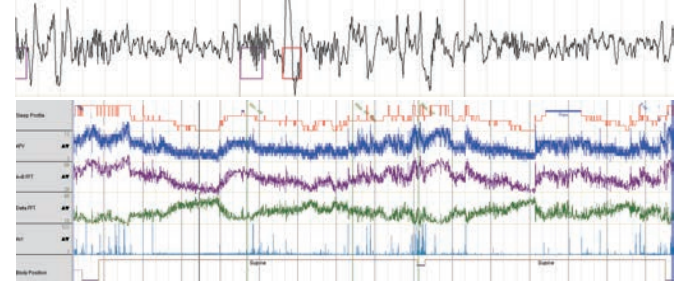

## Sleep Walking

**SOMNOWatch®** is an excellent device for detecting this sleep disorder, as up to 14 days of Body Position, Light, and Motor Activity can be recorded. The report discriminates between lying left, right, supine, prone, upright and walking.

FDA approved for adults only

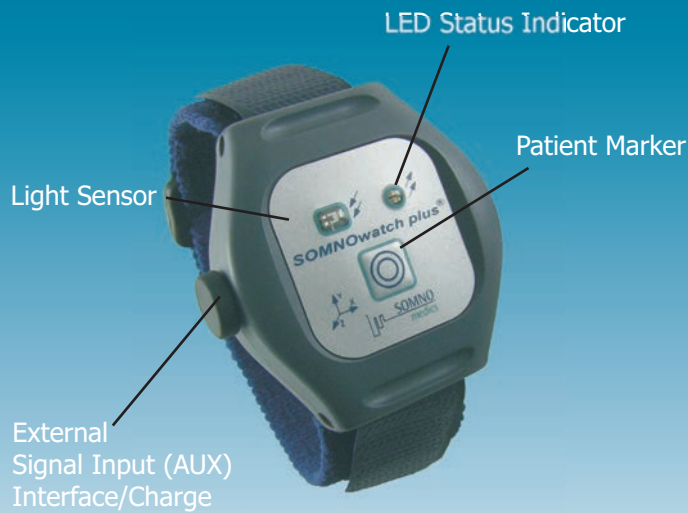

### 7 Channels

6 Internal (Body Position, 3 Activity Sensors (x,y,z - Axis), Ambient Light, Patient Marker)

1 External Signal Input (AUX)

### SENSORS FOR AUX

External Sensors	Pressure Sensor for Nasal (Oral) Flow + Snore
	Pressure Sensor for CPAP (0 to 15 cm H <sub>2</sub> O)
	EEG Electrode
	ECG Electrode
	PLM Electrode (EMG/ACTI)

### DATA PROCESSING

12 Bit ADC

Adjustable Sampling Rates - 128/s to 1/s

Adjustable Storage Rates - 1/120s to 128/s

Internal Data Storage 8/16 MB

Storage of Raw or Averaged Data User Selectable

### POWERSUPPLY

Li-Ion Battery, 630 mAh (rechargeable)

### SIZE & WEIGHT

45 mm Diameter x 16 mm, 30 g (incl. Battery)

### DEVICE FEATURES

Battery Charging During Data Transfer through USB Port

Programmable Start- and End-Times up to 20 Measurements

Device Status Indicator (Transferring, Recording, Standby)

Patient Marker Button

Waterproof

### SOFTWARE

Fast and Accurate Analysis and Scoring Software for:

Respiratory Analysis, PLM-Detection, Sleep, Wake, REM, Stage 1, 2, 3, 4, Tremor Analysis, EEG, Cardio Analysis

Editing of Events in the Raw Data

Computer aided Artefact Detection

Automatic Report and Form Letters

Data Base (Option - Compatible with SOMNOscreen®)

## Analysis of All Standard Signals

### Actigraphy

Sleep/Wake Detection and Sleep Efficiency (Time-in-Bed)  
Daily or Weekly Data Display  
REM/NREM Differentiation (ECG Option)  
REM, 1, 2, 3 and Stage 4 Differentiation (EEG Option)

### PLM

Computer aided Identification of PLM & LM Correlated to Body Position  
PLM-Index Distribution  
Quantification of the Motor Activity for RLS  
Correlation of Cortical Micro Arousals (EEG Option)

### Respiratory Screener

Apnoea/Hypopnoea Detection  
Snore Detection  
Body Position Correlation

### EEG

1-Channel EEG, up to 18 Hours  
FFT Module for Sequential Frequency Analysis of the Raw Data  
Spectral Analysis of Alpha, Beta, Delta and the Averaged Frequency Value (AVF)  
Micro Arousal Analysis According to the ASDA-Criteria  
Sleep Fragmentation  
Artefact Detection

### ECG

1-Channel ECG, up to 18 Hours  
Recognition of Brady/Tachycardia and Arrhythmia  
Heart Rate Variability (HRV)  
Sympatho-Vagal Balance (SVB)


### Tremor Analysis

Identification of Tremor Frequency & Tremor Intensity  
Motion Efficiency

### Actigraphy (Exercise, Sport, Rehabilitation)

Evaluation of Exercise Periods  
Correlation of the Motor Activity and the Heart Frequency

## Example of Respiratory Analysis

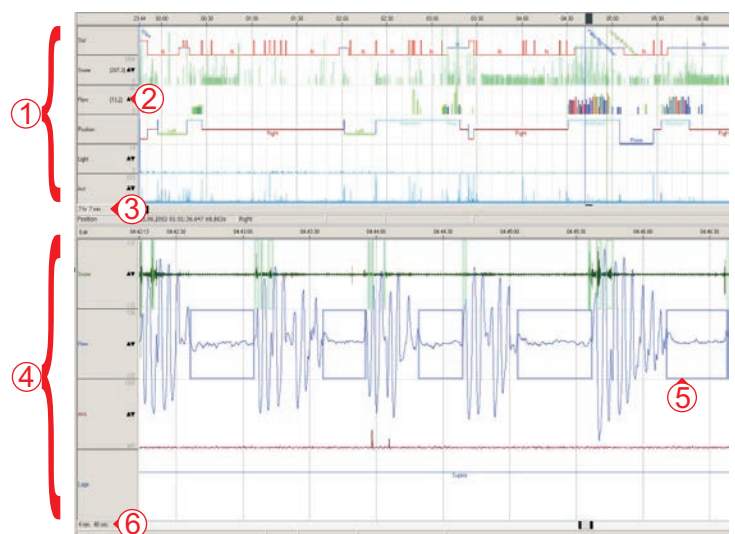

- (1) Analysis Data
- (2) Index per Hour
- (3) Analysis Time-Base Data
- (4) Raw Data
- (5) Events
- (6) Raw Data Time-Base

The system provides fully quick and easy manual editing. All events are colour coded and displayed in the Raw Data View.

## Application/Configuration

Actigraphy Sleep/Wake	Actigraphy Training/Sport	PLM Recorder	Movement Analyser	Respiratory Screener	REM/NR Recorder	Long-term Body Position	Long-term ECG	Long-term EEG
Non-Dominant Arm	Arm - Leg Body	Leg	Arm - Leg	Thorax	Thorax	Thorax	Thorax	Thorax

Signals / Sensors		Application/Configuration								
		Actigraphy Sleep/Wake	Actigraphy Training/Sport	PLM Recorder	Movement Analyser	Respiratory Screener	REM/NR Recorder	Long-term Body Position	Long-term ECG	Long-term EEG
Internal	Body Position	● <sup>(*)</sup>	●	●	●	●	●	●	●	●
	Movement	● <sup>(1)</sup>	●	● <sup>(1)</sup>	● <sup>(2)</sup>	● <sup>(1)</sup>	● <sup>(1)</sup>	● <sup>(1)</sup>	● <sup>(1)</sup>	—
	Ambient Light	●	●	●	●	●	●	●	●	●
	Button Marker	●	●	●	●	●	●	●	●	●
External	Flow & Snore	○	○	○	○	●	—	○	—	—
	ECG	○	○	○	○	—	●	○	●	—
	EEG	○	○	○	○	—	—	○	—	●
	CPAP	○	○	○	○	—	—	○	—	—
	PLM - EMG or ACTI	○	○	○	○	—	—	○	—	—

● Standard ○ Option ●<sup>(\*)</sup> Position ●<sup>(1)</sup> Quantitative Recording ●<sup>(2)</sup> x, y, z - Axis



### 7 Channels

6 Internal (Body Position, 3 Activity Sensors (x,y,z - Axis), Ambient Light, Patient Marker)

1 External Signal Input (AUX)

### SENSORS FOR AUX

External Sensors  
 Pressure Sensor for Nasal (Oral) Flow + Snore  
 Pressure Sensor for CPAP (0 to 15 cm H<sub>2</sub>O)  
 EEG Electrode  
 ECG Electrode  
 PLM Electrode (EMG/ACTI)

### DATA PROCESSING

12 Bit ADC

Adjustable Sampling Rates - 128/s to 1/s

Adjustable Storage Rates - 1/120s to 128/s

Internal Data Storage 8/16 MB

Storage of Raw or Averaged Data User Selectable

### POWERSUPPLY

Li-Ion Battery, 630 mAh (rechargeable)

### SIZE & WEIGHT

45 mm Diameter x 16 mm, 30 g (incl. Battery)

### DEVICE FEATURES

Battery Charging During Data Transfer through USB Port

Programmable Start- and End-Times up to 20 Measurements

Device Status Indicator (Transferring, Recording, Standby)

Patient Marker Button

Waterproof

### SOFTWARE

Fast and Accurate Analysis and Scoring Software for:

Respiratory Analysis, PLM-Detection, Sleep, Wake, REM, Stage 1, 2, 3, 4, Tremor Analysis, EEG, Cardio Analysis

Editing of Events in the Raw Data

Computer aided Artefact Detection

Comprehensive Reports and Form Letters

Data Base (Option - Compatible with SOMNOScreen®)

DISTRIBUTED BY : **Hitwin Healthcare Pvt. Ltd.**

7/10, Jaganathan Nagar 2nd Main Road,  
Arumbakkam, Chennai, India - 600106.

Ph: 91 44 4684 5555 (20 Lines), 91 44 4233 3313

Mob: 91 93441 66778

**FDA approved for adults only**

[www.hitwinhealthcare.com](http://www.hitwinhealthcare.com)